MEDICAL

SONITA MEDIC

SURGICAL

SUPPLIES

Anaesthetics Division

Adjustable Prone Head Support System

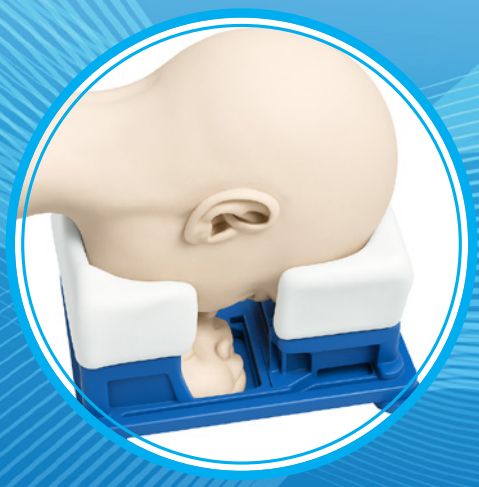

| www.sonitamedic.com.au |

- EMAIL: customers@sonitamedic.com.au
- PHONE: 1800 SONITA (766 482)
- MOBILE: 0423 178 332

SYDNEY :
Suite 242 / 60
Walker St, North Sydney,
NSW 2060

MELBOURNE :
Suite 10 / 327 Clarendon St,
South Melbourne,
VIC 3205

BRISBANE :
524 Old Bay Road
Burpengary East,
QLD 4505

PERTH
Suite 76 Ground Floor
50, St Georges Terrace,
Perth WA 6000

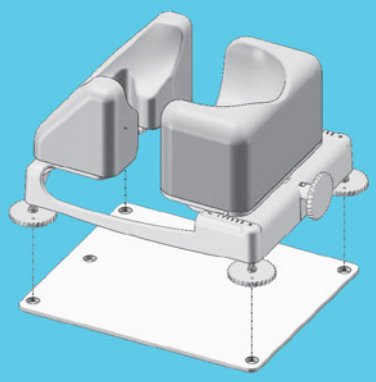

- Easy set-up
- Fully adjustable cushion set
- Enhanced patient stability
- Improved visibility of patient's eyes & ET Tube
- Latex Free

Product Features:

- Fully adjustable prone head pads.
- Adjustable Range for height: 0-28mm
- Adjustable Range for distance between Disapoable Foam Pads: 15-70mm

Applications

To support and protect face in the prone position surgeries, facilitating anaesthesia intubation, keeping smooth breathing.

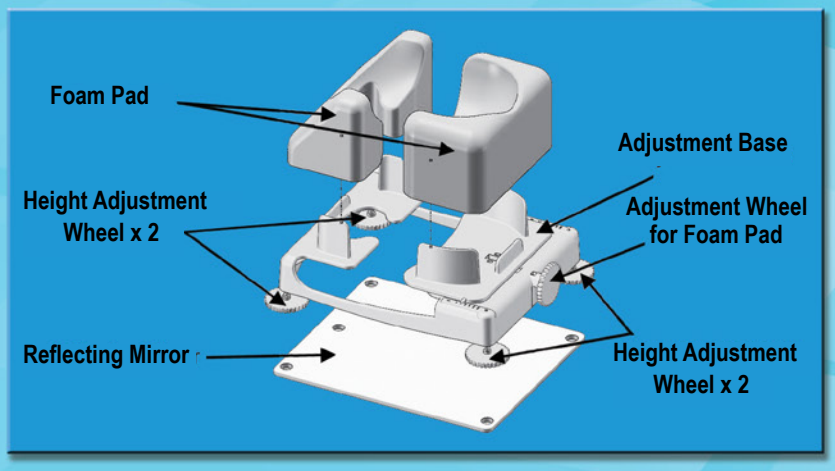

How to operate:

1. Put the reflecting mirror on the operating table. Insert the disposable foam pads on the adjustment base.
2. Put the adjustment base on top of the relecting mirror, making sure the base secured in the holes of the mirror. Turn the adjustment wheel for foam pad to position the foam pads as needed.
3. Position the patient on the disposable foam pads. Turn the height adjustment wheels to position the patient in desired height.
4. The foam pads are made of memory foam, being comfortable, pressure distributing, disposable, clean and requires no sterilisation.

Adjustable Prone Head Pad

Most desirable solution for pressure management of face and head in prone position surgeries

Code	Description	Unit of Measure
• **AM-FC-1101-17**	Reusable Adjustable Prone Head Pad Base & Mirror	Each
• **AM-FC-1101-18**	Disposable Foam Cushion Set for AM-FC-1101-17	Box of 12
• **AM-FC-1101-18-5**	Disposable Foam Cushion Set for AM-FC-1101-17	Box of 5
• **AM-FC-1101-18-6**	Disposable Foam Cushion Set for AM-FC-1101-17	Box of 6
• **AM-FC-1101-18-Single**	Disposable Foam Cushion Set for AM-FC-1101-17	Each

SONITA MEDIC MEDICAL SURGICAL SUPPLIES
■ PHONE: 1800 SONITA (766 482) ■ MOBILE: 0423 178 332
■ EMAIL: customers@sonitamedic.com.au ■ WEB: www.sonitamedic.com.au
■ OFFICE's in: . SYDNEY . MELBOURNE . BRISBANE . PERTH

This Adjustable Prone Head Support System is designed for use during surgeries in the prone position, providing clinicians with improved visibility of the patient's face.

Instructions:

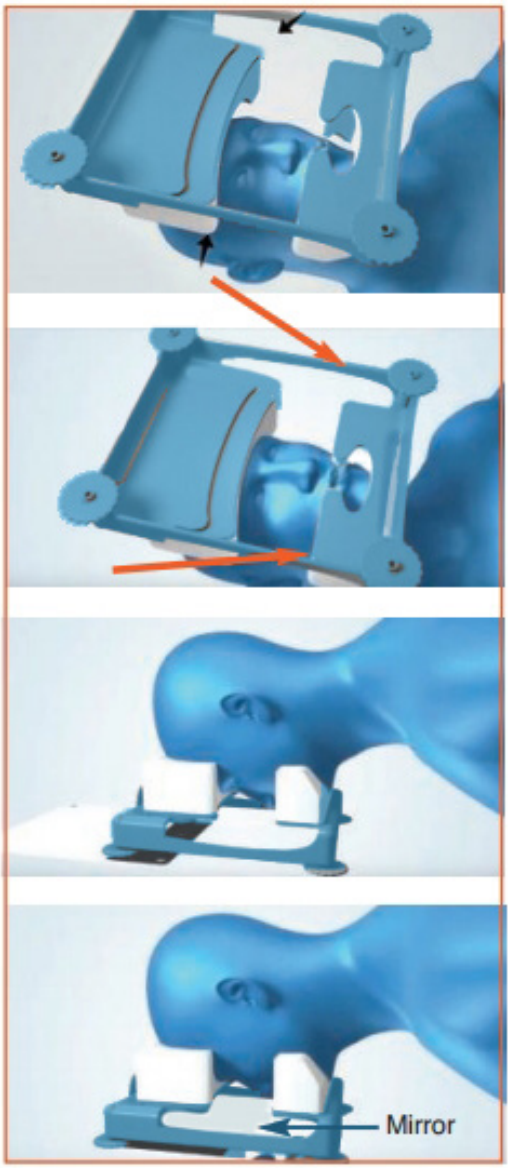

STEP 1

While the patient is supine, position the Adjustable Prone Head Support System with cushions over the patient's face, ensuring the eyebrows remain visible and the ET tube is not kinked.
Note the depth of the ET tube before turning the patient.
During the transition to the prone position, securely hold the head support system and cushion set in place on the patient's face.

STEP 2

Clinicians can use the sides of the Adjustable Prone Head Support System frame as handles to securely hold the base while turning the patient.

STEP 3

After turning the patient to the prone position, verify the depth of the ET tube, then slide the mirror underneath and align the feet of the Adjustable Prone Head Support System base with the inserts on the mirror.

STEP 4

Adjust the foam cushions and feet of the system to ensure a proper fit and maintain neutral spinal alignment. If needed, reposition the patient's body to achieve a neutral neck position. Level the base by adjusting the feet of the Adjustable Prone Head Support System. Finally, connect the anesthesia circuit to the ET tube.

STEP 5

Once the patient is in position, verify that the face and cushions are properly aligned, ensuring the face and eyes are centered within the cushion opening and there is sufficient space between the nose and the mirror.
Ensure the ET tube and any other devices are not kinked or obstructing the view of the eyes.
Regularly reassess the eyes, nose, and neck to confirm they remain correctly positioned.

IMPORTANT WARNINGS:

1. Failure to maintain a neutral neck position may lead to neck injury and/or chin abrasions.
2. To help prevent skin abrasions and pressure ulcers, frequently assess the patient's face and reposition the head at intervals recommended by your department's protocols or clinical guidelines.
****Standard practice typically recommends repositioning every two hours.*

SONITA MEDICAL SURGICAL SUPPLIES
■ PHONE: 1800 SONITA (766 482) ■ MOBILE: 0423 178 332
■ EMAIL: customers@sonitamedic.com.au ■ WEB: www.sonitamedic.com.au
■ OFFICE's in: . SYDNEY . MELBOURNE . BRISBANE . PERTH